

INVESTIGATION OF MECHANICAL AND BIOMEDICAL PROPERTIES OF NEW DENTAL ALLOY WITH HIGH CONTENT OF Au

VOJKAN LAZIĆ¹, DRAGOSLAV STAMENKOVIĆ¹,
ALEKSANDAR TODOROVIĆ¹, REBEKA RUDOLF², IVAN ANŽEL²

¹University of Belgrade, School of Dentistry, Clinic for Prosthodontics, Belgrade,
²University of Maribor, Faculty for Mechanical Engineering, Maribor, Slovenija

ABSTRACT

The basis for developing a new dental alloy with high Au content is appropriate chemical composition and manufacturing technology. The demands which have to be met when developing a new dental alloy are linked with fulfilling the necessary requirements for making the alloy suitable for use in metal-ceramic restorations. Due to the stress generated by masticatory forces, alloys for dental restorations must have corresponding mechanical properties (yield strength, tensile strength, and elongation), hardness, the coefficient of thermal expansion (CTE), and biocompatibility. Namely dental alloy placed in an oral cavity reacts with the environment and deteriorates.

New dental alloy with high Au content is based on the ternary system of Au-Pt-Zn with a nominal composition of 86.9Au-9.9Pt-1.5Zn, and about 1,5 wt.% micro-alloying elements (In, Ir, Rh). The dental alloy was melted and cast in a vacuum-induction melting furnace in Zlatarna Celje.

The results analyses of different heat-treated states showed that the optimal mechanical properties and hardness of an Au-Pt-Zn alloy can be reached with combinations of heat treatment for 20 minutes at 723 K and then slowly cooling, if the alloy was annealed at 1223 K for 30 minutes and the water quenched. Research results confirmed that the microstructure of the Au-Pt-Zn alloy consists of two phases: a₁-phase rich in Au (main phase) and a₂-phase rich in Pt (minor phase). During XRD analysis and use of the Rietveld method, it was found that the a₁-phase content is about 98,5 wt.% while the content of a₂-phase is 1,5 wt.%. STA analyses show that the Au-Pt-Zn alloy has a solidus temperature of about 1292 K and a liquidus temperature of about 1412 K.

The optical properties of Au-dental alloy were investigated by means of spectrophotometric colourimetry. Spectral reflectance data from the mirror-polished flat samples of initial Au dental alloy were collected under the CIE standard illuminant D65.

Finally the test of cytotoxicity of new Au based dental alloys using standard *in vitro* assays for testing the biocompatibility with establishing new, more sensitive, *in vitro* tests on cell lines was done.

According to the results of our research we can conclude that new dental alloy from Zlatarna Celje satisfied all requested standards regarding mechanical properties, hardness and CTE: R_{p0}=550 [N/mm²], R_m=610 [N/mm²], A= 9%, 180 HV and CTE (25-600°C) about 14,45×10⁻⁶K⁻¹. This new Au dental alloy has a yellow tinge in comparison to conventional Au-Pt-Zn alloys and did not show cytotoxicity when using standard short-term *in-vitro* assays on an L929 cell.

Key words: Au dental alloy, characterisation, microstructure, properties

1. INTRODUCTION

Gold alloys have been used in dentistry, not only because their gold colour is preferred, but also because they have extremely high chemical stability in the mouth, plus several desirable mechanical properties such as high strength, ductility and elasticity (1). They contain five or more elements, the essential components of the alloys being gold and platinum. The main specific physical requirements for those dental alloys used for porcelain fused to metal (PFM) technique are: a) a melting range starting at no less than 1100 °C, b) a coefficient of thermal expansion closely matched to that of high-fusing-point dental porcelain (960-980 °C) developed for the PFM technique – the values for these coefficients should stay within the ranges $12.7\text{-}14.8 \times 10^{-6} \text{ K}^{-1}$ for the alloys, and $10.8\text{-}14.6 \times 10^{-6} \text{ K}^{-1}$ for porcelain, c) minimal creep or sag when firing the porcelain, d) good wetting of alloy by the porcelain, e) tensile strength about 600 N/mm² and yield strength about 550 N/mm², f) hardness about 180 HV and g) elongation about 10 %. On the other hand, gold alloy for casting would have a melting range as low as possible whilst an Au alloy for porcelain veneers would have a solidus temperature around 100 °C higher than the firing temperature of the used porcelain, in order to ensure that the cast framework does not sag during firing.

Among various types of alloys for PMF restorations, the Au-Pt-Zn-based high noble alloys have the advantage of being around for some considerable time. They are part of clinical experience and are extremely successful (2). The bond between the ceramic and the metal, in particular, is very strong and highly reliable (3). Accordingly for our new Au dental alloy we selected a combination of the following alloying elements: Au, Pt, Zn and traces of: Ir, In, Rh. We wanted to keep all the favourable properties of gold and to improve its inadequate strength and hardness by Pt, Zn and Ir alloying (4). When considering the formulations of Au-Pt-Zn-based high noble alloys for porcelain bonding, high Au contents are required to ensure biocompatibility and large Pt concentrations are necessary to sufficiently raise the melting range above the porcelain firing temperature to prevent distortion during porcelain application (2,3). By the addition of Zn we wanted to lower the surface tension of the liquid alloy, thus enabling the material to be cast into very thin sections. The zinc also serves as a dezoxidant, together with Ir and In. This is because of their affinity to oxygen, being the first to react with it and thus, protect other metals from oxidation. Other micro-alloying metals are added also to form a thin oxide film at the surface of the alloy during the porcelain firing cycle (5,6). This new alloy has no Ag which easily reacts with oxygen, gives porous castings, forms sulphur compounds, and can lead to tarnishing and ceramic discoloration (greening). This new Au alloy also has no palladium or copper. Pd reacts with hydrogen; it gives porous castings and can cause allergic reactions. Cu gives reddish colour to an alloy, it reacts with oxygen and forms copper-oxide on the alloy's surface, which can cause ceramic discoloration. These are the reasons for the selected chemical composition of the alloy: about 88.5 w.% Au, 8.7 w.% Pt, 1.5 w.% Zn, and 1.3 w.% of different micro-alloying elements (Ir, In < 0.5 w.%, Rh). Micro-alloying elements are necessary for precipitation hardening; small

additions of iridium can reduce the grain size of the alloy, while the presence of rhodium enhance both strength and colour (4).

Testing of our new Au dental alloy included examining the solution treated and heat treated alloy. Measurements of hardness were done according to standard 6507-1:1998, and static tensile testing was performed for determination of the mechanical properties.

Dental alloys used in dentistry must also have good biocompatibility which concerns the biological acceptability and biological performance of those materials used in dentistry. Moreover, biocompatibility has been equated with the lack of a significant interaction between materials and tissues. It has been documented *in vitro* and *in vivo* that metallic dental devices release metal ions, mainly due to corrosion. These metallic components may be locally and systemically distributed and could play a role in the aetiology of oral and systemic pathological conditions. The quality and quantity of the released cations depend upon the type of alloy and various corrosion parameters. Prosthodontic restorations remain in an oral environment for many years and are exposed to the corrosive influences of saliva, temperature changes, pH changes, etc. Metals in electrolyte (saliva) release ions can lead to oxidative processes which tarnish and precipitate the metal in the surrounding tissues (7). Until now no general correlation has been observed between alloy nobility and corrosion. Dental cast alloys very often cause local adverse tissue reactions such as gingivitis and periodontitis, due to the release of metal ions into the surrounding microenvironment. Their cytotoxic effects are well documented using different *in vitro* and *in vivo* assays. This was the reason why less cytotoxic or non-cytotoxic precious noble-metal alloys with a high content of gold (Au) and platinum (Pt) although more expensive, are introduced in dental practice. In this study, only the parts of *in vitro* biocompatibility tests were performed. Within this study we tested the cytotoxicity of our new Au-Pt-Zn dental alloys using standard *in vitro* assays and to establish new, more sensitive, (*in vitro*) tests on cell lines.

In addition to the extremely successful clinical experiments, the attraction of Au-Pt-Zn-based high noble alloys is with the yellow colour. Nowadays it is suggested that colour control must be taken into account as one of the criteria when manufacturing dental gold alloys for crown and bridge metal-ceramic restorations. It has been claimed that a high gold content means that the alloys impart a warm, dentin-like colour to the ceramics. Because of this feature, there is a complete elimination of gingival 'black line disease' associated with traditional metal-ceramic fixed restorations. The optical properties of our new Au-dental alloy were investigated by means of spectrophotometric colourimetry.

2. EKSPERIMENTAL WORK

The melting of very pure components (Au=99.99 w.%, Pt=99.99 w.%, Zn=99.99 w.%, In=99.99 w.%, Rh=99.99 w.%, Ir=99.99 w.%) were performed at Zlatarna Celje d.d. in vacuum-induction melting furnace at vacuum $p=10^{-2}$ mbar and temperature $T=1400^{\circ}\text{C}$. Casting of the melted alloy was performed under argon pressure above 1,03 bar in a metal cast with diameter 8 mm (8). The alloy ingot was followed with

subsequent thermo-mechanical treatment (procedures of profile and polish milling, thermal treatment) and cutting-off the strip to form a regular shape. Alloy specimens were first solution-treated at 950°C for 30 min and quenched using water. The solution treated samples were then subjected to heat treatments which were carried-out in a tube furnace at selected temperatures (400°C, 450°C and 500°C) for different times (10 min, 20 min, 30 min) and, finally, slowly cooled to room temperature.

Testing of the new Au dental alloy included examining the solution treated and heat treated condition. Measurements of hardness were carried out according to standard 6507-1:1998, with the Vickers test on the Zwick 3212 microhardness measurement device. For testing the samples, we used applied load $F=49$ N, according to standard. For every sample, we performed 12 measurements.

The static tensile testing using tensile device Zwick/Roell ZO 10 was performed for determining the mechanical properties. Measurements of mechanical properties for the all states were performed in one series with 6 samples. The research conditions, as well as the shapes and dimensions of the tensile test tubes were according to standard SIST EN 1562:2000 (chapter 6.2). Tests were performed under constant speed of increasing deformation $v=1.5$ mm/min. Tensile test tubes were cast and then cut-out from the cylinder shaped casting (diameter 3 mm).

Measurements of the thermal expansion coefficient (CTE) was performed in one series which consisted of 3 samples, on the Mechanical Dilatometry device (at the Chair for Engineering Materials at Faculty of natural sciences and engineering, University of Ljubljana).

For the microscopic analysis, dental alloy plates were ground and then polished using different polish pastes. The samples were, after metallographic preparation, cleaned in an ultrasound vibration cleaning device (medium alcohol). Those specimens for optical microscopy were then etched in $H_2O-H_2O_2-FeCl_3$ solution for 2 min at room temperatures. Concurrently those polished specimens for electron microscopy were put in the chamber of the Sirion NC 400 scanning electron microscope, with vacuum of 10^{-10} mbar. Sirion FEG is a high-resolution scanning electron microscope with field emission gun (FEG) which enables the observation and analysis of nano-scale particles. Microscopic analysis includes examination of the polished surface and qualitative and quantitative micro-chemical analysis at characteristic points on the dental alloy. We observed surfaces using an electron beam voltage at 30 kV, and over different working distances (6.5 mm, 7.2 mm, etc.).

XRD analysis was carried-out to determine the phase compositions of the Au-Pt-Zn alloy. The diffraction patterns of both alloys were collected on a PANalytical X'pert PRO MPD diffractometer using reflection geometry and $CuK_{\alpha 1}$ radiation. The 2-theta range was from 30 ° to 120 °. Diffraction patterns were compared using the X'Pert HighScore (PANalytical) computer program. The Crystallographica Search Match (Oxford Cryosystems) program was applied for qualitative phase analysis. The database used by the program was PDF-4 (9). Crystallographic data of the identified phases were retrieved from the ICSD database (10,11). Quantitative phase analysis was performed using the Topas (Bruker AXS) program, which uses the Rietveld method (12,13).

For the biocompatibility (cytotoxicity) test, disk-shaped specimens (4 mm × 4 mm and 10 mm × 10 mm) from Au dental alloys were prepared using a conventional lost-wax technique which simulates the preparation of the cast metal alloy for clinical use. The disks were polished and rinsed in distilled water. After cleaning by sonification for 5 minutes, the samples were autoclaved. Large disks were cultivated in a medium for cell cultures (RPMI medium + 10 % fetal calf serum) for 8 days, in order to test the cytotoxic effect of metals released from alloys (alloy-media), whereas small disks were used for testing the direct cytotoxic effect. Controls consisted of inert glass samples, pre-treated as test samples. Standard cytotoxicity assays were performed on L929 fibroblast cells according to ISO standards: ISO 10993-5; 1992(E) and ISO 7405; 1997(E). These procedures included morphological examinations of cells cultivated with dental alloys for 24h, and quantification of cell death by Tripan blue dye exclusion. In addition, the succinic dehydrogenase (SDH) activity was measured using the MTT assay. Optimization of these assays included prolonged incubation of cells with test samples for 7 days or a combination of direct and indirect (alloy-media) effects. New assays included proliferation of rat spleen lymphocytes in the presence of concanavalin A (Con A), and different concentrations of alloy - media, measured by ³H-thymidine incorporation, and apoptosis of thymocytes and splenocytes using morphological examinations, and staining with propidium iodide or merocyanine 540.

For spectrophotometric colourimetry, the polished samples of new Au dental alloy were mounted on a disk shaped specimen (10 mm × 10 mm × 10 mm), and spectral reflectance data under the CIE standard illuminant D65 were collected at 10 nm intervals (D65/10) in wavelengths ranging from 400 to 700 nm. These measurements were done on a Spectraflash SF 600 Plus spectrophotometer and repeated 3 times, rotating the sample by 120 degree each time. Three-dimensional colour coordinates lightness L^* , chromaticity indices a^* (red green direction) and b^* (yellow-blue direction) in the CIE $L^*a^*b^*$ system, and chroma, C^* and hue angle h in the CIE L^*C^*h system were obtain to specify the sample colour. The CIELAB colour difference parameter DE^* between two samples was evaluated. For reference-sample 1 used a comparatively old Au dental alloy with nominal composition Au: 85.9 w.%, Pt: 11.7 w.%, Zn 1.1 w.% and about 1.3 w.% micro-alloying elements (In, Ir, Rh) and for sample 2 a new Au dental alloy with nominal composition was used: about 88.5 w.% Au, 8.7 w.% Pt, 1.5 w.% Zn, and 1.3 w.% of different micro-alloying elements (Ir, In, Rh) see Figure 1.

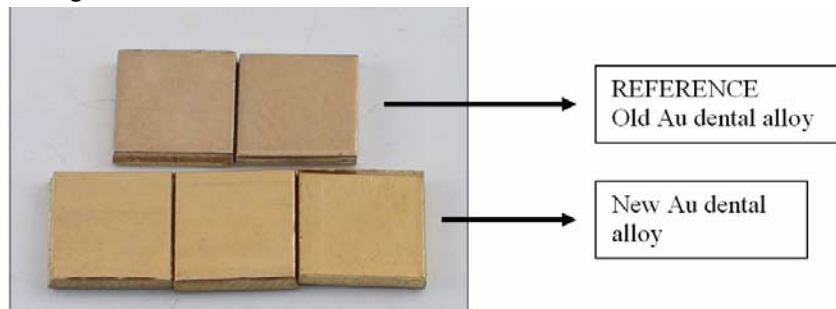


Figure 1: Old and new Au-Pt-Zn alloy specimens for testing optical properties

3. RESULTS

The average results of the hardness measurement are presented in Table 1 for each alloy state. For the solution-treated specimen, the average hardness value was about 125 HV. It can be concluded that the alloy a solution-treated state had very low hardness. On the other hand there were different heat treated samples where hardness began to increase and reached the maximum value at isothermal holding by 450 °C for 20 min and also 30 min (the results in Table 1 are grey coloured).

Table 1: Results of hardness measurements [in HV5]

| Solution treated state : | | |
|---|---|---|
| 125 | | |
| Heat treated at 400 °C for 10 min: 145 | Heat treated at 400 °C for 20 min: 170 | Heat treated at 400 °C for 30 min: 175 |
| Heat treated at 450 °C for 10 min: 160 | Heat treated at 450 °C for 20 min: 180 | Heat treated at 450 °C for 30 min: 180 |
| Heat treated at 500 °C for 10 min: 160 | Heat treated at 500 °C for 20 min: 168 | Heat treated at 500 °C for 30 min: 170 |

The average results of the mechanical properties measurements (yield strength at 0.2 % strain, tensile strength and elongation) for all tensile test tubes are gathered in Table 2. With respect to the results for hardness, we can conclude that this optimal mechanical property also applied the samples of Au dental alloy which had been heat treated at 450 °C for 20 min (grey coloured). These samples fulfil, after heat treatment, all the necessary standards regarding mechanical properties and hardness.

Table 2: The average value of the mechanical properties measurements

| | $R_{p0.2}$ [N/mm ²] | R_m [N/mm ²] | A [%] |
|----------------------|---------------------------------|----------------------------|-------|
| Initial hom. state | 340 | 390 | 15 |
| HT 400 °C, 10 min | 450 | 520 | 9 |
| HT 400 °C, 20 min | 470 | 530 | 13 |
| HT 400 °C, 30 min | 500 | 560 | 12 |
| HT 450 °C, 10 min | 520 | 580 | 10 |
| HT 450 °C, 20 min | 550 | 610 | 9 |
| HT 450 °C, 30 min | 550 | 610 | 10 |
| HT 500 °C, 10 min | 520 | 570 | 10 |
| HT 500 °C, 20 min | 540 | 600 | 10 |
| HT 500 °C, 30 min | 550 | 600 | 13 |

Measurements of the thermal expansion (CTE) coefficient have shown that the average value of CTE (25-600 °C) for Au-Pt-Zn alloy is about $14.45 \times 10^{-6} \text{ K}^{-1}$.

The results of the chemical spectral analysis of new Au dental alloy are present in Table 3 in w.% or in at.%.

Table 3: The average value of the chemical spectral analysis of Au-Pt-Zn dental alloy

| Element | Weight % | Atomic % |
|---------|----------|----------|
| Zn K | 1.55 | 4.48 |
| Rh L | 0.39 | 0.63 |
| In L | 0.49 | 0.89 |
| Ir L | 0.39 | 0.39 |
| Pt L | 8.67 | 8.42 |
| Au L | 88.51 | 85.19 |
| | | |
| Totals | 100.00 | 100.00 |

Detailed optical microstructural examination of the annealed (Figure 2a) and heat-treated (Figure 2b) Au-Pt-Zn dental alloys with optimal mechanical properties (Au-Pt-Zn-OP) reveal that its microstructure contains two different phases: the base matrix which is identified as an Au-rich α_1 -phase, and an other phase, which appears to be small particles and is known as a Pt-rich α_2 -phase (6). The grain sizes of the α_2 phases are large as, in reality (approximately between 2-8 μm); it is a consequence of the sample's metallographic preparation (especially the influence of the etching process). Optical microscopy shows that the α_1 -phase has approximately equal sizes in the annealed and heat-treated states, which is different from α_2 -phase. The size and density of α_2 -phase namely change according to the condition of the heat treatment (temperature and time). Generally the higher temperature of the heat treatment leads to larger particles of α_2 -phase. The growth of α_2 -phase is in parabolic function of time which means that, after some time, particle growth stops. Examinations showed that the microstructure became homogeneous with the performing of heat treatment. α_2 -phase (in the form of small particles) is located at the grain boundaries and within the grains. We envisage that the optimal and most homogeneous distribution and size of α_2 -phase particles was achieved by the Au-Pt-Zn-OP sample which was heat treated at $T = 723 \text{ K}$ for $t = 20 \text{ min}$ after solution treatment.

Further phase assumptions were confirmed by EDX analysis. The gained average EDX results on the Au-Pt-Zn-OP samples show that the α_1 -phase has about 87.32 wt.% Au, 10.58 wt.% Pt, 1.00 wt.% Zn; Ir, In and Rh are traceable ($< 1 \text{ wt.}\%$). On the other hand, the α_2 -phase in this sample contains about 75.64 wt.% Pt, 19.62 wt.% Au, 4.2 wt.% Rh, In and Zn are traceable, while in this phase no Ir was detected.

An X-ray powder diffraction curve with a combination of the Rietveld plot for the Au-Pt-Zn-OP alloy is shown in Figure 3. Measured diffraction pattern (circles) is compared to the calculated one (thin solid line), which is composed of the two

components: α_1 (major) and α_2 (minor). The contribution of the latter is shown with the solid thick line at the bottom.

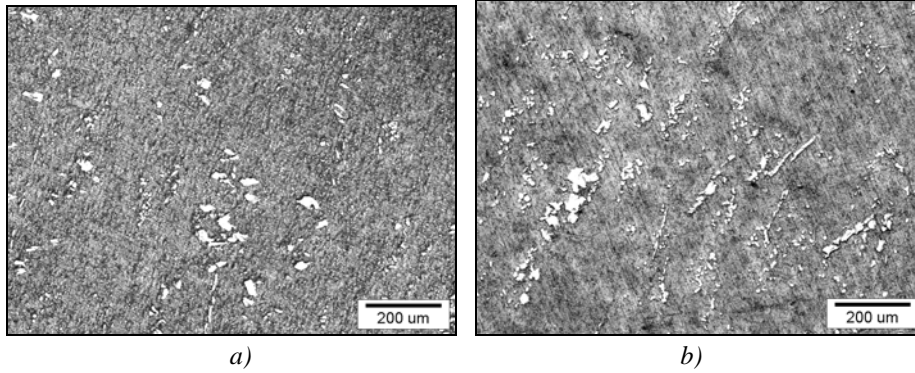


Figure 2. The optical microstructure of Au-Pt-Zn alloy after: a) solution treatment at 1223 K for 30 min and water quenched, b) heat treatment at 723 K for 20 min and slowly cooled to the T_{room} .

In addition the main phase, the Au-Pt-Zn-OP alloy contains only one minor phase (its characteristic peaks are visible, for example, at diffraction angles of 39,7, 46,3, 67,1 degrees). Qualitative phase analysis of the Au-Pt-Zn-OP alloy revealed that the major α_1 -phase is similar to gold (PDF card 4-784 for pure gold specifies a cubic unit cell with a parameter of 0.40778 nm); minor α_2 -phase is similar to platinum (PDF card 4-802 specifies a cubic unit cell with the parameter of 0.39231 nm).

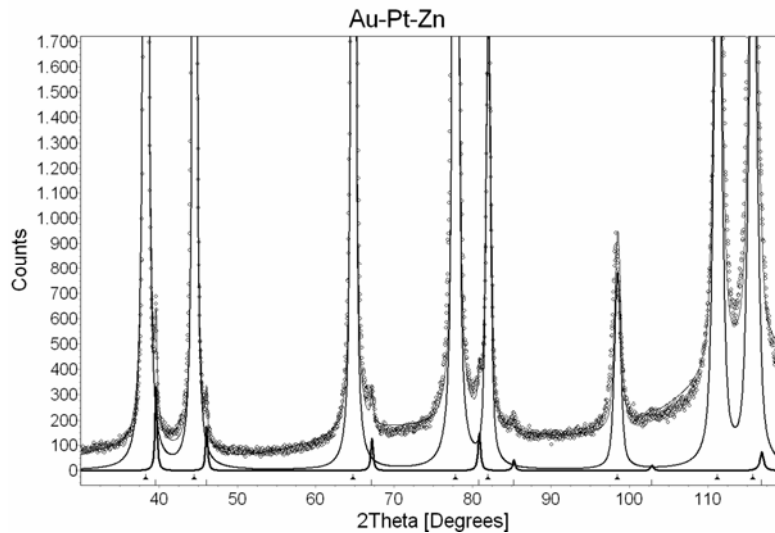


Figure 3. Rietveld plot for the Au-Pt-Zn-OP alloy. Measured diffraction pattern (circles) is compared to the calculated one (thin solid line), which is composed of the two components: alpha1 (major, 98.4 %) and alpha2 (minor, 1.6 %). The contribution of the latter is shown with the solid thick line at the bottom.

The mass ratio of the two phases was determined by the Rietveld method. In the Au-Pt-Zn-OP alloy, there is about 98,5 wt.% of the major phase α_1 and about 1,5 wt.% of the minor phase α_2 . Rietveld method also enables the determination of the unit cell parameters. The unit cell parameter of phase α_1 is 0.4068 nm, while the unit cell parameter of the α_2 phase is 0.3941 nm. Beside the peaks belonging to these two phases, there is no additional peak present in the pattern of the Au-Pt-Zn-OP alloy.

Standard cytotoxic tests showed that Au-Pt-Zn alloy has not cytotoxicity after short term (24 h) incubation of L929 cells. Prolonged incubation of cells with dental alloys showed that Au-Pt-Zn decreased the SDH activity in L929 cells by only 15.1 ± 6.2 % (the difference was not statistically significant) compared to control glass material. Similar results were obtained using the combination of alloys and alloy-media. The Au-Pt-Zn alloy did not induce apoptosis of rat thymocytes and splenocytes during a 24 h assay. However, alloy - media significantly suppressed the proliferation of rat splenocytes in the culture. Inhibition depended on the concentrations of alloy media. Au-medium was less suppressive (26.3 ± 4.6 %; $p < 0.05$ compared to glass-medium). When examining apoptosis in cultures of Con A-stimulated splenocytes, we observed apoptosis of splenocytes incubated with Au-medium at level 49.1 ± 3.0 % ($p > 0.05$; NS).

Figure 4 shows a spectral-reflectance curve and Figure 5 represents the chromaticity a^* , b^* indices of CIELAB colour space for the new Au-Pt-Zn against comparable old alloys. Table 4 shows the comparison of colour coordinates for the reference old Au-Pt-Zn alloy and the new Au-Pt-Zn alloy, and their colour difference ΔE^* .

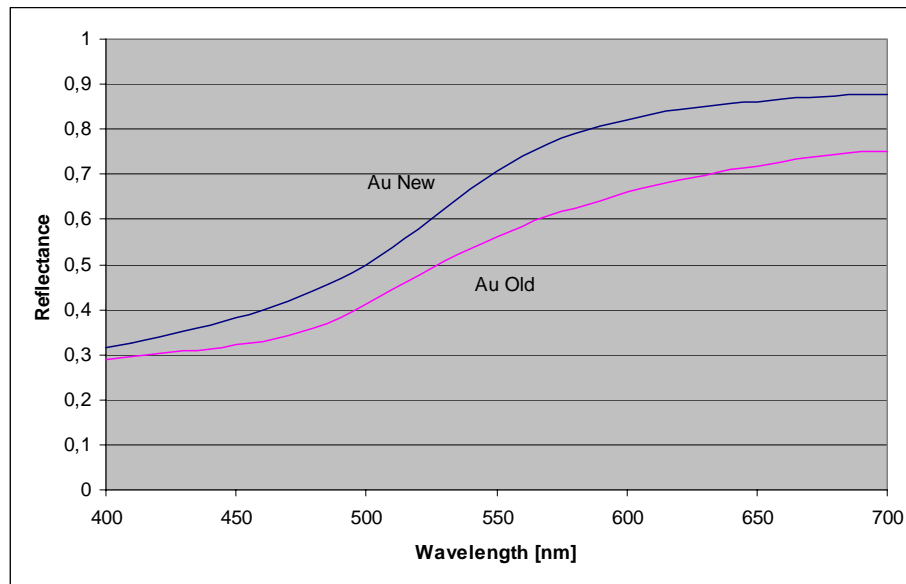
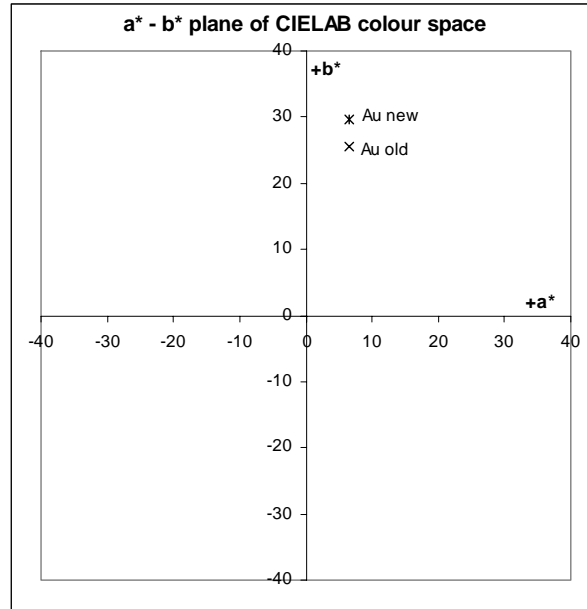


Figure 4: Spectral reflectance curves for both Au-Pt-Zn alloys

Table 4: Colour coordinates (standard illuminant D65/10)

| Alloy | L* | a* | b* | DE* | Batch is |
|----------------------------|-------|------|-------|-------|----------|
| Reference: old Au-Pt-Zn | 78.97 | 6.64 | 25.62 | | |
| New Au-Pt-Zn | 86.06 | 6.43 | 29.62 | 8.137 | yellow |

Figure 5: a^* and b^* plane of CIELAB colour space

4. DISCUSSION

The present studies of heat treatment's influence on the mechanical properties of a newly- produced Au-Pt-Zn alloy show improvement in hardness, yield strength at 0.2% strain, and tensile strength during processing. These results indicate that the specimen which was heat-treated for 20 minutes at 723 K after solid solution treatment had maximum hardness and tensile strength. The reasons for these conclusions are the chemical composition of the Au-Pt-Zn alloy, microstructure formation and, consequently, the strengthening effect which occurred during heat treatment.

The Au-Pt-Zn alloy is characterized by the unknown ternary Au-Pt-Zn system. According to the obtained results and the revealed microstructure with known α_1 and α_2 phase contents the most important marginal phase diagram.

The Au-Pt binary phase diagram contains a miscibility gap (Au) + (Pt), the critical point of which is about 61 at.% Pt and at 1533 K. Miscibility gap occurs in the solid solution field, as well as the controversial form of the liquidus and solidus boundaries. The immiscibility is well-known for the Au-Pt system in a solid state. After casting, a

solid solution nucleates from the melt. During cooling the alloy enters the miscibility gap separating into Au-rich and Pt-rich phases. With heat treatment at 1223 K the alloy enters the single phase zone between the miscibility gap and the solidus line (14). At this temperature, a solid solution is thermodynamically stable with random distribution of the atoms within the crystal lattice (6). The inhomogeneous texture formed after casting, therefore, is thermodynamically unstable. Owing to high energy, the atoms could diffuse in the crystal lattice and be forced to distribute randomly on the atomic sites. Subsequently, the alloy became homogeneous. Then during the cooling process, the homogenized microstructure kept in balance. But a small amount of the Pt-rich phase could still precipitate from the solid solution, depending on the cooling rate. Thus, all the specimens showed a microstructure composed of, not only α_1 -phase, but some α_2 -phase too. In the solution treatment process at 1223 K combined with water quenching, many crystal defects remained and supersaturated solid solution was achieved. After this treatment the alloy was thermodynamically in a metastable state. When metastable, specimens were put under different heat treatment temperatures they were subjected to isothermal treatment; precipitation reactions occurring driven diffusion (15).

In the case of heat treatment at 723 K for 20 minutes the precipitation reaction for α_2 phase was optimal regarding to their size and distribution (16). The measured micro-hardness of single phase has namely shown that α_2 phase has 4 times higher value as the α_1 phase. In this case we could presume that the α_2 phase is reinforced elements and the α_1 phase the matrix, similar to the conditions for the composite material. We supposed the α_2 phase is the main factor responsible for strengthening Au-Pt-Zn alloys according to the researched microstructure (17,18). Homogeneous distribution, higher density and the size of α_2 phase particles clearly lead to higher values for the hardness and mechanical properties of the Au-Pt-Zn alloy. In this case we can't forget the solution strengthening of the α_1 -phase with the elements Pt, Zn, Rh, which is consequently reflected in the higher hardness value (90 HV) compared to the pure gold (≈ 60 HV) (18).

Based on the results of this study, for the practical application of the present Au-Pt-Zn alloy, it is advisable to perform heat treatment.

According to the results Au-Pt-Zn OP did not show cytotoxicity using standard short term in vitro assays on L929 cell. However, prolonged cell incubation did not reveal the adverse effect of Au-Pt-Zn-OP alloy on L929 cells manifested by reduced SDH activity and also did not show pro-apoptotic effect on rat thymocytes and splenocytes in culture, but significantly decreased Con A - stimulated proliferation of these cells.

The optical properties investigations show that our new Au-Pt-Zn alloy has yellow colour compared with the old alloy with less Au content. It seems that the difference of Au at value 2.6 w.% for total chemical composition of the alloy has an influence on the colour difference parameter DE^* cca 8.1. Since the DE^* value of 1.0 is said to be just discernible by the average human eye (19), the colour of the new dental alloys may be very well-distinguished from that of the referenced old alloy. With the analysis of spectral reflectance curves for both Au-Pt-Zn alloy it is shown, that the new Au-Pt-Zn

alloy has a higher reflectance of about 10 % in those wavelengths ranging from 400 to 700 nm. On the other hand in the CIE $L^*a^*b^*$ system chromaticity indices a^* for both alloys is equally comparable, while the indice b^* of the new alloy has a higher value for about 4 units. This is the reason that new Au-Pt-Zn alloy is yellower than the old. The yellow colour on the surface plays an important role in developing the restoration aesthetics (20). Although the alloy is covered with successive layers of porcelain, light travels through the porcelain and is reflected back out. If the surface of the alloy is silver (white) in colour then the entire light spectrum is reflected out. This includes the blue region which, when passing through the pink gum tissue, produces a dark unsightly outline. Au-Pt-Zn dental alloy is opaque and highly reflective, the perceived colour is determined by wavelength distribution of the radiation, which is reflected and not absorbed (19). Material possessing a much higher reflectivity for the low-energy end of the visible spectrum (red and yellow light) than for the other parts of the spectrum will have a reddish to yellow colour (20).

5. CONCLUSIONS

1. From the results of our examinations, we can conclude that the Au-Pt-Zn dental alloy from Zlatarna Celje fulfils all the requested standards in the sense of mechanical properties and hardness. The obtained results for this alloy are: $R_{p0.2} = 550 \text{ N/mm}^2$, $R_m = 610 \text{ N/mm}^2$, $A = 9 \%$, 180 HV.

2. The analyses of different heat-treated states show that the above-mentioned mechanical properties and hardness of the Au-Pt-Zn alloy can be reached with combinations of heat treatment for 20 minutes at 723 K and slowly cooling after that, if the alloy was annealed at 1223 K for 30 min and water quenched.

3. The microstructure of the Au-Pt-Zn alloy consists of two phases: α_1 -phase rich in Au and α_2 -phase rich in Pt. It was found that the number and density of α_2 -phase increased by the performing of heat treatment. α_2 -phase is in the form of small particles (2-8 μm) and is located at the grain boundaries, and within the grains. The α_2 -phase shows value about 340 HV and are the main factor for the strengthening of the Au-Pt-Zn alloy.

4. The growth of α_2 -phase is in parabolic function heat treatment time and higher temperature of HT leads to more and larger particles of α_2 -phase. The optimal and most homogeneous distribution and size of α_2 -phase particles was achieved in the Au-Pt-Zn-OP sample.

5. The gained EDX results on the Au-Pt-Zn samples with the optimal mechanical properties show that the α_1 -phase has approximately 87.32 wt.% Au, 10.58 wt.% Pt, 1.00 wt.% Zn; Ir, In and Rh are traceable (< 1 wt.%). On the other hand, the α_2 -phase contains about 75.64 wt.% Pt, 19.62 wt.% Au, 4.2 wt.% Rh, In and Zn are traceable, while in this phase no Ir was detected.

6. Using the XRD analysis and Rietveld method, it is calculated that in the Au-Pt-Zn-OP alloy contain about 98.5 wt.% of the major phase α_1 and about 1.5 wt.% of the minor phase α_2 .

7. The Au-Pt-Zn alloy did not show cytotoxicity when using standard short-term *in vitro* assays on L929 cell and prolonged cell incubation did not revealed any adverse effect on the L929 cells manifested by reduced SDH activity. The Au-Pt-Zn alloy did not show any pro-apoptotic effect on rat thymocytes and splenocytes in culture, and significantly decreased Con A - stimulated proliferation of these cells.

8. The optical property investigations show that our new Au-Pt-Zn alloy has yellower colour compared to the old alloy with less content of Au. It seems that the difference of Au at value 2.6 w.% in the total chemical composition of the alloy influences on the colour difference parameter DE^* cca 8.1, which may very clearly be distinguished from that of the referenced old alloy.

9. In the Au-Pt-Zn alloy we can't forget the solution strengthening of the α_1 -phase with the elements Pt, Zn, Rh which is, consequently, reflect in the higher hardness value (90 HV) compared to the pure gold (\approx 60 HV).

ACKNOWLEDGMENTS

Zlatarna Celje d.d. is working on the development of a new high Au content dental alloy with the support of associates from the Institute of Materials Technology, Faculty of Mechanical Engineering, University of Maribor; School of Dentistry, University of Belgrade, University of Ljubljana, Faculty of Natural Sciences and Engineering and Zlatarna Celje d.o.o. Belgrade. This paper is a part of Slovenian Applied Project no. L2-7096, Bilateral Project SLO/SR BI-CS/06-07-031 and EUREKA Programme E!3555 DEN-MAT. The authors gratefully acknowledge the Ministry of Higher Education, Science and Technology, and Slovenian Research Agency.

6. REFERENCES

- [1] WILLIAMS, D. (1990): *Medical & Dental materials*. Oxford OX3, England.
- [2] R. VAN NOORT (1994): *Introduction to Dental Materials*. Mosby, London, pp. 219-221.
- [3] GERMAN, R. M. (1980): *Journal of Dental Research*.; Vol. 59.
- [4] FISCHER, J. (2002): Effect of small additions of Ir on properties of a binary Au-Ti alloy. *Dental Materials*.; Vol. 18, No. 4, pp. 331-335.
- [5] KNOSP, H., HOLLIDAY, R.J., CORTI, C.W. (2003): *Gold Bulletin*.; No. 36, pp. 93-102.
- [6] WANG, J. N., LIU, W. B. (2006): A Pd- free high gold dental alloy for porcelain bonding. *Gold Bulletin*.; Vol. 36, No. 3.
- [7] HORNEZ, J. C., LEFVRE, A., JOLY, D. and HILDEBRAND H.F. (2002): Multiple parameter citotoxicity on dental alloys and pure metals. *Biomolecular Engineering*.; Vol. 19, pp. 103-117.
- [8] KRIZMAN, A., RUDOLF, R., ALBREHT, B. (2006): Melting and casting of dental alloys with high Au-content. *Livarski vestnik*.; Vol. 53; No. 1, pp. 19-31.

- [9] International Center for Diffraction Data, Release 2006.
<http://www.icdd.com/products/pdf4.html>.plus.
- [10] ICSD database (latest update 2007-1, FIZ Karlsruhe.
<http://www.fiz-karlsruhe.de/icds.html>.
- [11] H.M. Rietveld, *Acta Crystallographica.*, 21 (1966), A228, 78-81.
- [12] R.A. Young, *The Rietveld Method*, University Press, Oxford, 1993.
- [13] J.C. Taylor, *Rietveld made easy: a practical guide to the understanding of the method and successful phase quantifications*, Sietronics Pty, Canberra, 2001.
- [14] R. Rudolf, B. Albrecht, B. Kosec, A. Križman, *IRT 3000*, 1(2006) 4, 64-65 (in Slovene).
- [15] I. Anžel, A.C. Kneissl, L. Kosec, R.Rudolf, L. Gusel, *Zeitschrift fuer Metalkunde*, 94 (2003) 9, 993-1000.
- [16] C.J. Raub, D. Ott, *Gold Bulletin*, 16 (1983) 2, 46-51.
- [17] C.W. Corti, *Gold Bulletin*, 32 (1999) 2, 39-47.
- [18] R. Rudolf, T. Zupančič Hartner, *IRT 3000*, 1(2006) 4, 40-41 (in Slovene).
- [19] CALLISTER, W. D. (1985): *Materials Science and Engineering: An Introduction*. John Willey&Sons, Inc., New York, pp. 535-536.
- [20] SAEGER, K. E. and RODIES, J. (1977): *Gold Bulletin.*; Vol. 10.